

CT Department Work Flow Tip

Exam: 8th Floor iDT 16 Slice(CT2) Start Up and Shut Down Procedures




Power Down

1. Logout of application software.




2. Select *Shutdown* in Windows XP login window. This should eventually turn off Dell computer inside of computer cabinet.

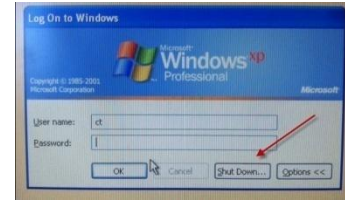

3. Next turnoff the CIRS computer. Open CIRS cabinet, and hold in for 15 secs. the black button on front of each of 2 computers. Order is not important. They should turn off within one-minute.



4. Turn OFF gantry at the CT control disc (desktop Frisbee).

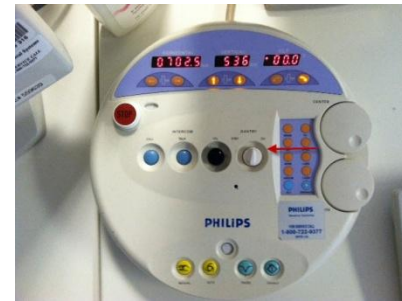

5. In back equipment room, pull down main breaker labeled CT3 on rear wall.



Power Up


1. In back equipment room, push up main breaker on rear wall.



2. It should NOT be necessary to reset the Teal Power Conditioner (cabinet below main breaker). Breaker lever inside should still be pointing to ON.



3.. Turn ON gantry at the CT control disc (desktop Frisbee). If there is power to the system there will be **red dots** showing in the **Vertical** and **Horizontal** positions. Turn on each of the two IRS computers by pressing black button on each one..

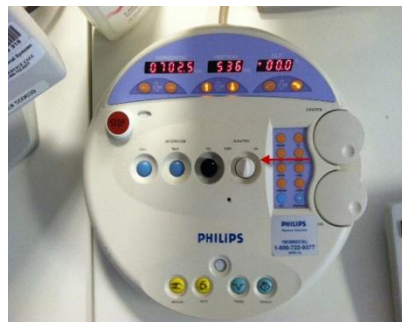


4. Turn on Dell computer (round button, upper right).




5. Logon the host computer using the default “CT”.



6. Accept License Agreement to proceed.



7. Perform Short Tube Conditioning, system will be ready in 3-5minutes.



Any Problems with Starting or Shutting down this system page the Philips Service for Help. After Hours contact the Philips Service desk at **1-800-722-9377**. Give them the Site ID for this Scanner, which is **226867**. Explain the situation and they will get someone to out to address the problem.

